


# COVID19+ 9G test™

## Diagnostic For Acute Respiratory Virus Testing

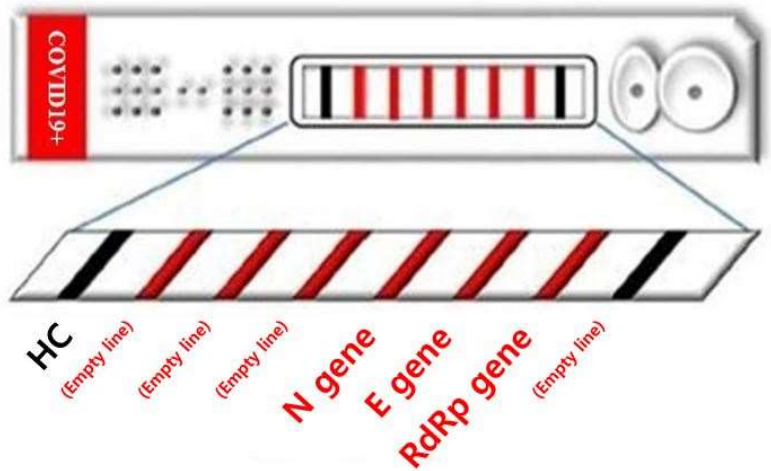

### ➤ 3 genes in 1 test

- Quick and easy test process
- Accurate results by targeting 3 genes
- Running time : 2 hrs 30 min


### ➤ Test Results

**Sample Type** Nasopharynx and throat smear, Sputum


**Package** 48 tests/kit

**Device** BMT 1D Scanner, BMT 9G-1000

#### COVID-19 Positive

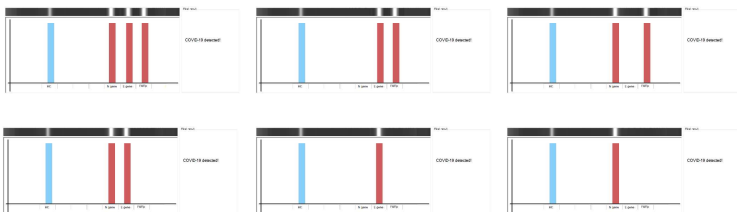

#### COVID-19 Suspected



#### Negative



## Easy to run tests and get reproducibility



#### Manual Method – BMT 1D Scanner™



#### Automation – BMT 9G-1000

24 tests result in 40 min

